



Desloratadine Assay with HPLC – AppNote

Alternate L1 Column used for HPLC Method of Desloratadine

This Desloratadine Assay is easily performed and the five injection overlay below demonstrates Run to Run consistency and Precision. The Peak Efficiency is very good and Peak Tailing guidelines are easily met with RSD values below 0.3%. This demonstrates a good alternate Column for your Desloratadine Method.

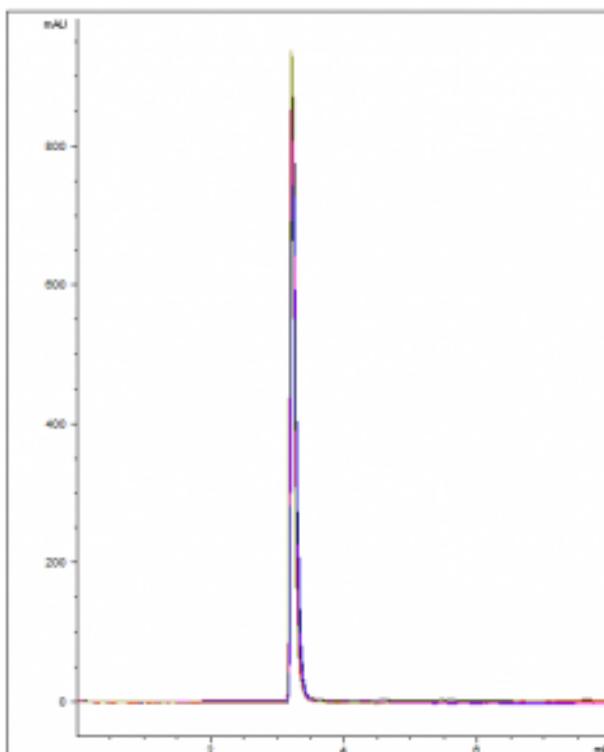

Peak:



Desloratadine

Met hod Conditions:

Column: Cogent Hyper Similar C18™, 5 um, 150Å

Catalog No.: [62518-25P](#)

Dimensions: 4.6 x 250 mm

Mobile Phase: 25:75 Acetonitrile / DI Water

Injection vol.: 2 μ L

Flow rate: 1.0mL / minute

Detection: UV @ 280 nm

Sample Preparation: Desloratadine 1.0 mg / mL in (50:50) Acetonitrile / DI Water

Note 1: Desloratadine is an antihistamine used to relieve allergy symptoms such as hives, watery eyes, runny nose, itching eyes/nose, sneezing, and itching.

Note 2: The Cogent Hyper Similar C18™ performs very similarly to the ThermoFisher® Hypersil BDS C18®.



Printed from the Chrom Resource Center

Copyright 2025, All Rights Apply

MicroSolv Technology Corporation

9158 Industrial Blvd. NE, Leland, NC 28451

Tel: (732) 380-8900

Fax: (910) 769-9435

Email: customers@mtc-usa.com

Website: www.mtc-usa.com