
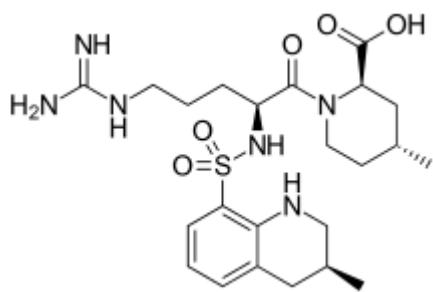


Peptide Argatroban Analyzed with HPLC - AppNote

A simple method for this di-peptide

A rapid, sensitive, and reproducible method has been developed for this blood thinner. The data below, (*an overlay of 10 chromatograms*) illustrates how the compound can be adequately retained and detected using this straightforward method.

A phenyl ring in the column stationary phase provides strategic use of π - π Interaction with the analyte making possible the use of a very simple, Mass Spec-friendly mobile phase with formic acid as an additive.

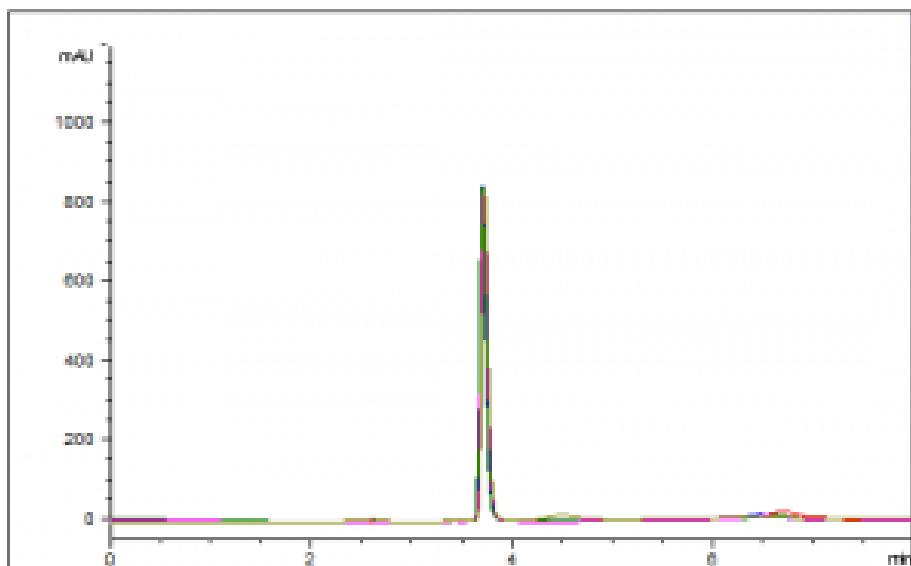

Peak:

Argatroban

Method Conditions

Column: Cogent Phenyl Hexyl™, 4µm, 100Å

Catalog No.: 68539-15P

Dimensions: 4.6mm x 150mm

Mobile Phase:

- A: DI water
- B: Acetonitrile

Time (minutes)	%B
0	25
1	25
3	50
4	50
5	25
8	25

Injection vol.: 2 μ L**Flow rate:** 1.0mL / minute**Detection:** UV @ 215nm**Sample Preparation:** 0.5 mg / mL in 50:50 acetonitrile / DI water**%RSD:** <1.0%**t₀:** 1.5 minutes**K':** 1.35

Notes : Argatroban is a synthetic direct thrombin inhibitor used for the prevention and treatment of thrombosis related to heparin use. It acts as a preventative of the formation of blood clots, which reduces the risk for stroke or other medical conditions.

Note 2 : Capacity is determined using the following equation: $k' = (t_R - t_0)/t_0$

- t_R = Retention time of an analyte peak
 - t_0 = Retention time of non-retained peak
-



Printed from the Chrom Resource Center

Copyright 2025, All Rights Apply

MicroSolv Technology Corporation

9158 Industrial Blvd. NE, Leland, NC 28451

Tel: (732) 380-8900

Fax: (910) 769-9435

Email: customers@mtc-usa.com

Website: www.mtc-usa.com