




Histamine and Methylhistamine Analyzed with LCMS - AppNote

No derivatization required for detection or retention with this method

Various assay methods for histamine (HA) and / or its metabolite, methylhistamine (MHA), in biological samples, have been developed. However, most of them require post-column (*for detection purposes*) or pre-column (*to achieve retention*) derivatization.

The method in this application note provides separation and detection of these two compounds yet doesn't require any derivatization. It is able to solve the inherently difficult problem of analyzing two biogenic amines with close physicochemical properties. A successful validation of the assay was indicated by the high linearity of calibration curves and the low inter- and intraday variation coefficients.

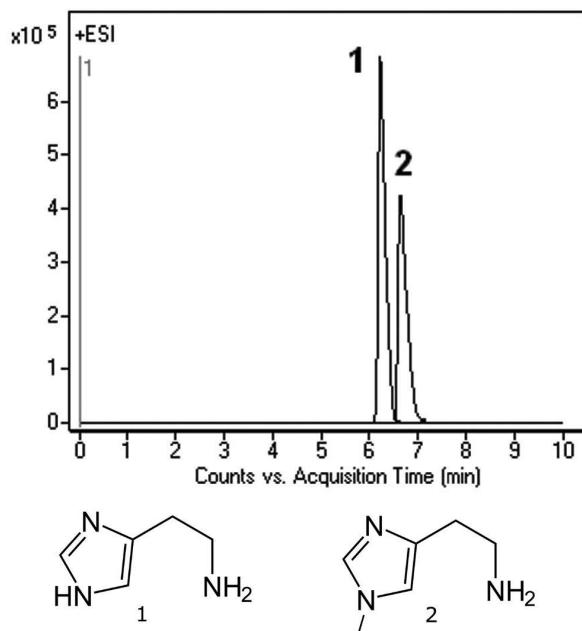

Peaks:

1. Histamine 112.0869 m/z [M+H]⁺
2. Methylhistamine 126.1026 m/z [M+H]⁺

Method Conditions

Column: Cogent Diamond Hydride™, 4µm, 100Å

Catalog No.: [70000-15P-2](#)

Dimensions: 2.1 x 150mm

Mobile Phase:

A: DI water with 0.1% formic acid (v/v)

B: Acetonitrile with 0.1% formic acid (v/v)

Gradient:

Time (minutes)	%B
0	70
2	65
6	10
8	10
9	70

Post Time: 2 minutes

Injection vol.: 1 μ L

Flow rate: 0.4mL / minute

Detection: ESI – POS - Agilent 6210 MSD TOF Mass Spectrometer

Sample Preparation: 1mg / mL of each compound was dissolved in DI water and filtered through a 0.45 μ m syringe filter (MICROSOLV Tech Corp). Sample for injection was diluted 1:100 with 50:50 solvent A / solvent B mixture.

t₀: 0.9 minutes



Attachment No 197 Histamine and methylhistamine analyzed with LCMS [Download File](#)

Printed from the Chrom Resource Center

Copyright 2025, All Rights Apply

MicroSolv Technology Corporation

9158 Industrial Blvd. NE, Leland, NC 28451

Tel: (732) 380-8900

Fax: (910) 769-9435

Email: customers@mtc-usa.com

Website: www.mtc-usa.com