





MDMA Analysis in Plasma Samples with LCMS - AppNote

Methylenedioxymethamphetamine Analyzed with MS

Click [HERE](#) for Column Ordering Information.

Under the described conditions, MDMA was retained and eluted as a Symmetrical Peak. The Sensitivity of the Method is very good and comparable to that reported with GCMS Detection [1]. Matrix effects were of minor extent and reproducible and hence should not compromise Quantification. The Method can be used for Forensic Research and Clinical Analysis.

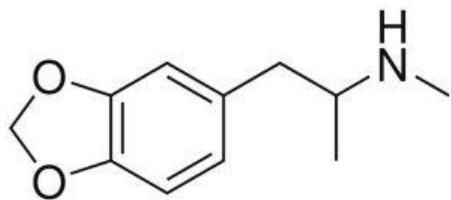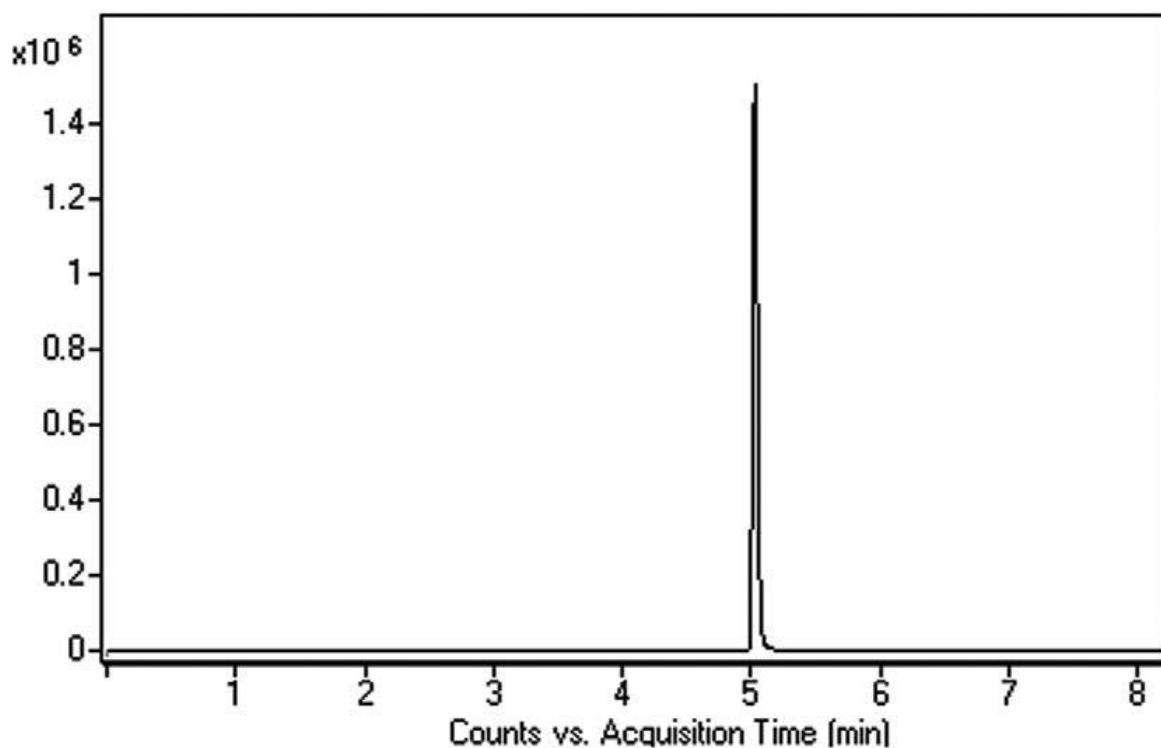

Peak:

(±)-3,4-Methylenedioxymethamphetamine, m/z 194.1176 [M+H]⁺

Method Conditions

Column: Cogent Phenyl Hydride™, 4 μ m, 100 \AA

Catalog No.: [69020-05P-2](#)

Dimensions: 2.1 x 50mm

Mobile Phase:

A: DI Water / 0.1% Formic Acid (v/v)

B: Acetonitrile / 0.1% Formic Acid (v/v)

Gradient:

Time (minutes)	%B
0	10
1	10
6	90
7	10

Post Time: 3 minutes

Flow rate: 0.4mL / minute

Injection vol.: 1 μ L

Sample Preparation: 50 μ L of Acetonitrile was mixed with 50 μ L of plasma for protein precipitation.

The samples were centrifuged (16000 \times g for 15 minutes), and the supernatant was filtered through a 0.45 μ m Nylon Syringe Filter (MICROSOLV Tech Corp.) and transferred to autosampler vials for injection.

Detection: ESI – POS - Agilent 6210 MSD TOF Mass Spectrometer

t₀: 0.9 minutes

Note: The Amphetamine derivative 3,4-methylenedioxymethamphetamine (MDMA), known also as Molly or Ecstasy, is often used or abused as a recreational drug. Because of a reported high inter-individual difference of its toxicity, sensitive analytical methods are needed. A urine test is a standard method to investigate drug abuse but the method has a very low diagnostic sensitivity and makes testing in plasma much more suitable.

Reference:

[1]. R. Kikura, Y. Nakahara, T. Mieczkowski, F. Tagliaro, *Forensic Sci. Int.* 84 (1997) 165–177.



Attachment No 263 Analysis of MDMA in Plasma Samples with LCMS pdf 0.2 Mb [Download File](#)

Printed from the Chrom Resource Center

Tel: (732) 380-8900

Copyright 2025, All Rights Apply

Fax: (910) 769-9435

MicroSolv Technology Corporation

Email: customers@mtc-usa.com

9158 Industrial Blvd. NE, Leland, NC 28451

Website: www.mtc-usa.com