




Peptide Synthetic, Analyzed with HPLC - AppNote

Peptide Production Confirmation Using the Cogent HPS[©] C18

An in-process Method for Qualifying a synthetic peptide is shown with 3 samples of tryptic "digests" were injected on the same Column. The Reproducibility from run to run on the samples is excellent giving the user a high level of confidence. The process and Method was further confirmed by coupling the HPLC Separation directory to Mass Spectrometry. The Mass data had a high degree of Accuracy and Reproducibility, verifying the peptide.

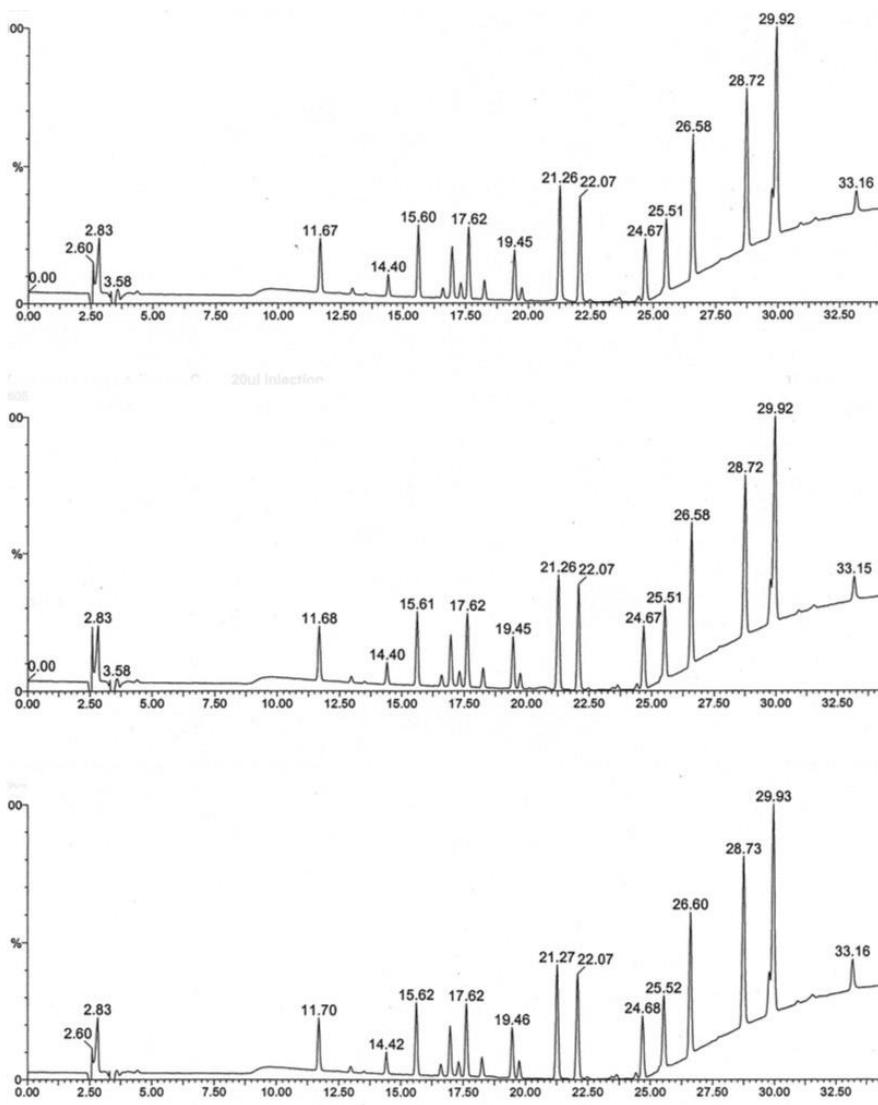

Method Conditions

Column: Cogent HPS C18TM, 5 μ m, 120 \AA

Catalog No.: [75018-25P](#)

Dimensions: 4.6 x 250mm

Mobile Phase:

A: DI Water with 0.1% Trifluoroacetic Acid (*TFA*)

B: Acetonitrile with 0.1% Trifluoroacetic Acid (*TFA*)

Gradient:

Time (minutes)	%B
0	0
20	60
20.1	0

Temperature: 30°C

Injection vol.: 20µL

Flow rate: 1mL / minute

Detection: UV @ 254nm

Sample Preparation: 3 Different Samples from the same peptide batch were digested using Trypsin and injected onto the HPLC Column.

Notes: Cogent HPS C18 Columns are perfectly suited for peptide analysis. The pore diameter, the exhaustive end capping and the low metal content of the Silica make these Columns an excellent choice for Peptide Mapping after digestion with Trypsin also known as a Tryptic Digest. Unique Selectivity and low cost make these Columns the choice of many Protein laboratories worldwide when Reproducibility and Reliability are mandatory.



Attachment No 16 Synthetic Peptide Production.pdf 0.2 Mb [Download File](#)

Printed from the Chrom Resource Center

Copyright 2025, All Rights Apply

MicroSolv Technology Corporation

9158 Industrial Blvd. NE, Leland, NC 28451

Tel: (732) 380-8900

Fax: (910) 769-9435

Email: customers@mtc-usa.com

Website: www.mtc-usa.com