

## PTFE that is Skived vs Cast in Headspace Septa Affecting Quantitation - Tech Information

Date: 30-MAY-2013 Last Updated: 5-FEBRUARY-2025

In headspace analysis, it is of utmost importance that a tight seal is formed between the septum of the cap and the vial. If there are even small gaps present in the seal, some of the analyte will escape through these gaps and lead to low recovery. In order to avoid problems of this kind, the quality of the septa should always be considered.

There are two manufacturing methods for PTFE used in headspace caps. The first method is **skiving**. In this technique, a long tube-shaped portion of PTFE material is mechanically cut at regular intervals to produce the circular septa discs used in the final headspace cap product. The second method is known as **casting**. Here the PTFE material is poured into molds in the shape of the headspace septa. Skiving is the cheaper of the two techniques because quality molds are expensive to manufacture. However, the skiving process is known to produce widespread defects in the material surface. On the edges of the material where the PTFE contacts the vial when sealed, these defects cause gaps in which volatile compounds may escape.

The difference in quality between these two septa types is readily apparent under magnification. Figure A below shows the PTFE side of a cast septum used in MICROSOLV Headspace Crimp Caps (catalog # 95025-07-1S). The surface here has only a few minor imperfections. In Figure B, the PTFE surface of a market leading skived headspace cap is shown. Here the surface has significant grooves all throughout the material. These grooves are the result of skiving techniques.

Figure A:

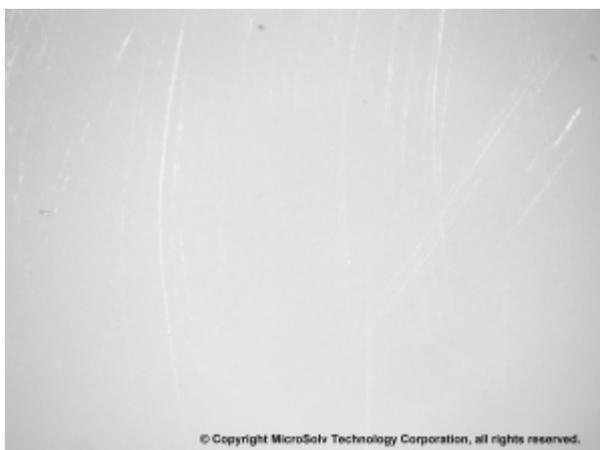


Figure B:



Printed from the Chrom Resource Center

Copyright 2025, All Rights Apply

**MicroSolv Technology Corporation**

9158 Industrial Blvd. NE, Leland, NC 28451

Tel: (732) 380-8900

Fax: (910) 769-9435

Email: [customers@mtc-usa.com](mailto:customers@mtc-usa.com)

Website: [www.mtc-usa.com](http://www.mtc-usa.com)